
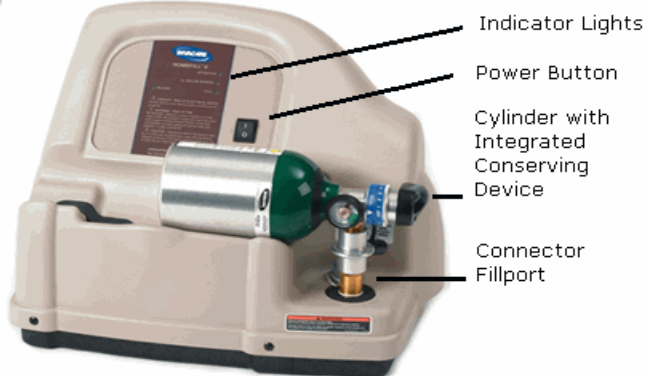


If you are experiencing issues with any oxygen device, please ensure that you are on your back-up oxygen cylinder prior to attempting any troubleshooting. Patients, who experience difficulty breathing or worsening of their medical condition, should contact their physician or 911 immediately.

The information provided in this publication is designed for general informational purposes only. It is not intended to be a substitute for professional medical advice, evaluation, diagnosis, services or treatment. You should not use this information to diagnose or treat any health problems or illnesses without consulting your physician. Please consult a doctor with any questions or concerns you might have regarding your medical condition and the urgency with which you may need to seek care for a particular condition.

Manufacturers user manuals for all devices are available on the manufacturer's website. Additional information can be accessed at apria.com/find-product-info/.

Product Description	Troubleshooting Questions
<p>HOME TRANSFILL (HTF)</p>   <p>Labels for the top diagram: Homefill Unit, Inlet Fitting, Interconnect Hose, Outlet Fitting, Homefill Stand, Concentrator.</p> <p>Labels for the bottom diagram: Indicator Lights, Power Button, Cylinder with Integrated Conserving Device, Connector Fillport.</p>	<p>No Power – Machine will not turn on/No Lights</p> <ul style="list-style-type: none"> • Is the unit turned on? • Is the unit plugged into a working outlet? • If the outlet is controlled by a wall switch, is the switch in the ON position? <p>No Air Flow or Low Air Flow</p> <ul style="list-style-type: none"> • Is the tubing kinked or obstructed? Ensure that all connections between the Concentrator and the HTF are tight and secure. • With the concentrator running, is the flow meter set above zero LPM and below 3 LPM? • Is the concentrator's inlet filter clean? (A clogged inlet filter may cause overheating.) Clean the filter as necessary. <p>Indicator Lights are on / Machine is alarming</p> <ul style="list-style-type: none"> • RED Light • If cylinder is full - remove cylinder, turn the unit off and attach an empty cylinder • Ensure that the cylinder is properly connected – turn the unit off, remove cylinder, reconnect cylinder and then turn the unit back on • Check all hoses to ensure they are secure • YELLOW Light • Ensure the concentrator has been on for at least 20 minutes so that it can warm up. If it hasn't been at least 20 minutes, turn off the HTF until it has been 20 minutes • Ensure all hoses are secure. Turn off the HTF for at least 10 seconds and then turn back on